

MetroLab Calibration


Environmental Conditions History

Area: Lab 1 - Electrical | Last 7 days | Generated 6/16/2026, 6:48:47 AM
Limits - Temp 19.0 to 21.0 C RH 40.0 to 60.0 % Pressure 980.0 to 1040.0 hPa


9 readings | 1 out of limits | Temp avg 20.5 (19.9 to 21.3) C

Time	Temp C	RH %	Pressure	OK?	Source	Recorded by
2026-06-07 20:43	20.6	54.3	1011.1	OK	MANUAL	Jane Doe
2026-06-07 19:43	20.5	53.5	1011.5	OK	MANUAL	Jane Doe
2026-06-07 18:43	21.3	52.6	1011.9	OUT	MANUAL	Jane Doe
2026-06-07 17:43	20.8	55.0	1012.0	OK	MANUAL	Jane Doe
2026-06-07 16:43	19.9	56.1	1010.8	OK	AUTO	Logger
2026-06-07 15:43	20.2	54.3	1011.3	OK	AUTO	Logger
2026-06-07 14:43	20.6	53.0	1011.7	OK	MANUAL	Jane Doe
2026-06-07 13:43	20.5	54.8	1011.2	OK	MANUAL	Jane Doe
2026-06-07 12:43	20.3	55.2	1011.6	OK	AUTO	Logger

Temperature (°C)

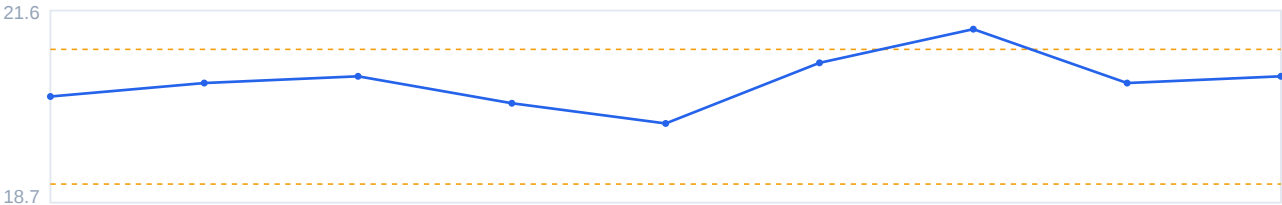

Humidity (%RH)

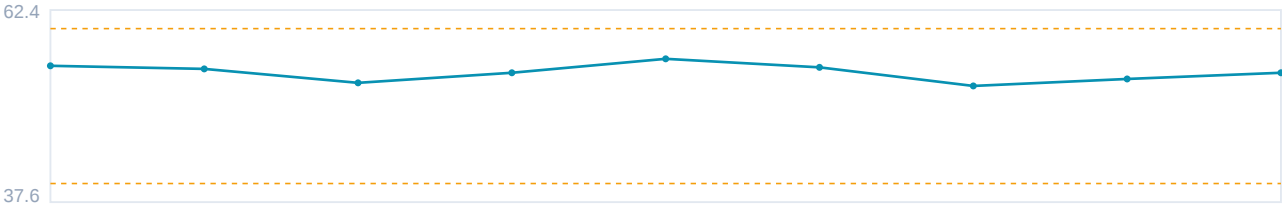

Atmospheric Pressure (hPa)

